

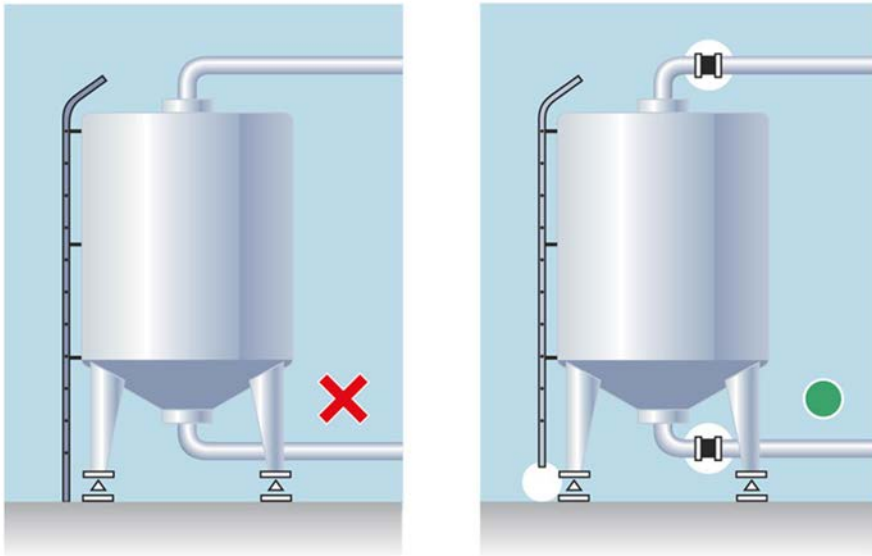


Example of LOAD MODULE orientation

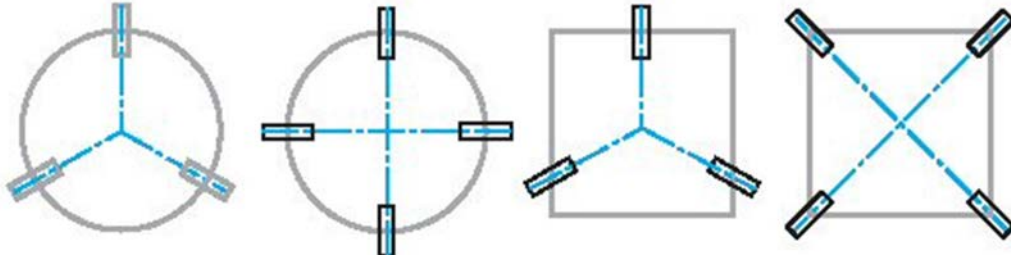

To achieve good weighing results, always use flexible connections to the vessel and check that no ladders or other arrangements connect the weighed vessel to surrounding foundation, walls or roof.

Advices for mounting KIMD-1 and KOM-1

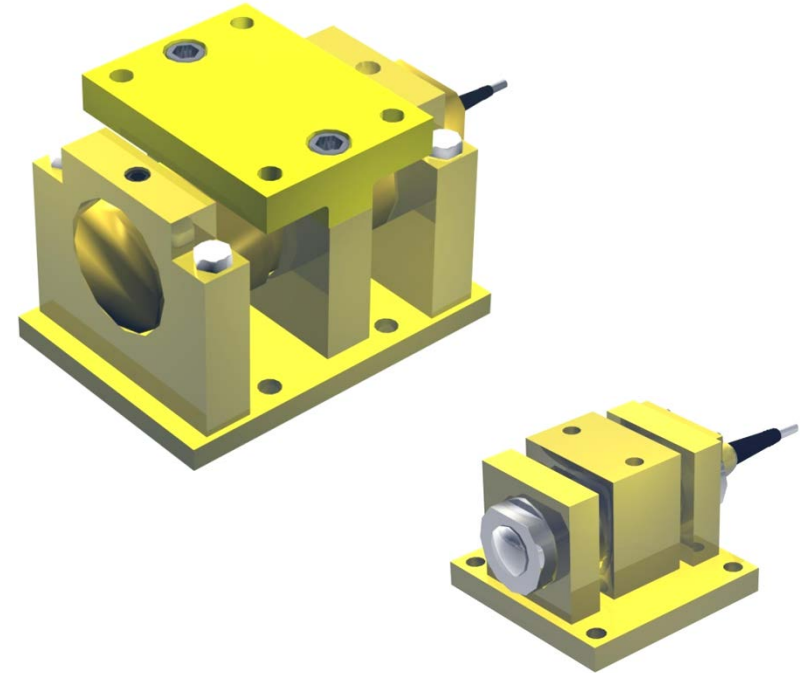


Vishay Nobel AB

Box 423, SE-691 27 Karlskoga, Sweden
Phone +46 586 63000, Fax +46 586 63099
e-mail: pw.se@vishaypg.com
www.weighingsolutions.com

Document no. 35126
Publication 850 205 R1
© Vishay Nobel AB, 2010-07-28
Subject to changes without notice.




1

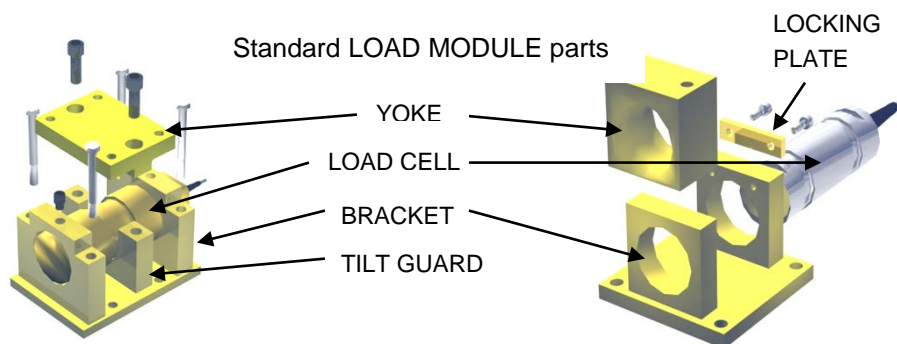

Assemble LOAD CELL, BRACKET, and YOKE to one LOAD MODULE.


2

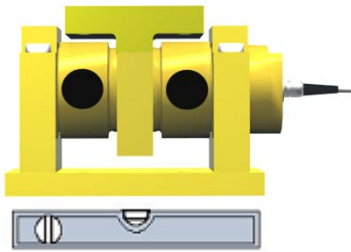

Level the LOAD MODULE within $\pm 1^\circ$ in both directions.

3


Recommended loading point. Check measure "x" between BRACKET and YOKE.

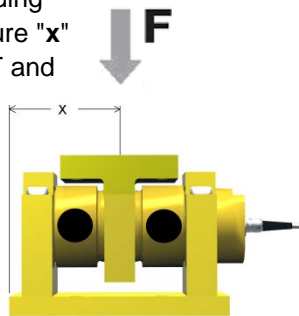

KIMD-1		KOM-1	
(mm)	X (mm)		x
		10 kN	37
		20 kN	37
		50 kN	65
		100 kN	60
		200 kN	70
500 kN	140	500 kN	125
800 kN	140		


4

Observe loading point position relative surrounding mechanical construction. It is very important that this is strong and must be rigid enough.

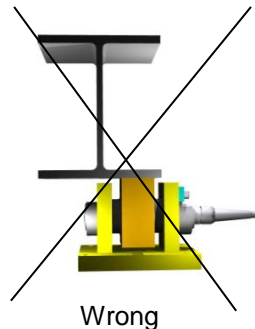

5


Check that there is a lateral play between YOKE and LOAD CELL by making sure that it is aligned with the LOAD CELL.

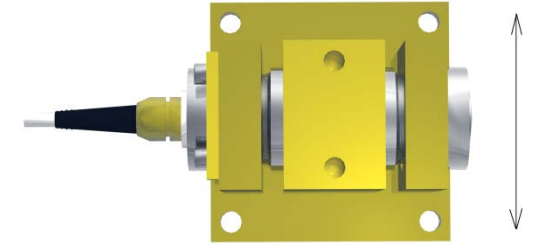

6

Attach YOKES under the vessel supports and position the vessel on the LOAD MODULES. Observe that the bedding should be horizontal.

Mark the hole pattern and drill. Mount the bolts; re-position the LOAD MODULES and the vessel.

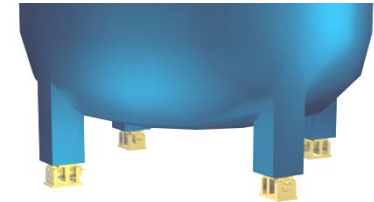

7

Check again the measure "x" between BRACKET and YOKE, and that the lateral play between YOKE and LOAD CELL is preserved.

For installations with four LOAD MODULES or more, the LOAD CELL output signals should be checked. Add shims between vessel support and YOKE to achieve similar signal levels.

8

Important notices:

IMPORTANT! WHEN DELIVERED THE MODULES ARE ONLY MOUNTED FOR TRANSPORTATION!

Tighten all bolts and nuts according to engineering standards.

Do not perform any welding with the LOAD MODULE in place.